PRODUCT BULLETIN

Product(s):	Narkomed 6000
Bulletin Number:	093
Release Date:	November 21, 2000
Pages:	2

Subject: Low Flow Wizard

Available with software versions 1.05 & higher is the low flow wizard—a tool that utilizes input from the DIVAN to qualitatively assess the amount of fresh gas surplus in a low flow case. This tool will help to ensure that fresh gas flow rates are at levels that minimize waste while satisfying set ventilation parameters.

This indicator incorporates a graphical representation of the fresh gas surplus, a message display area, and a help key (question mark) that invokes a test message when touched. The graph contains three areas: one for no surplus (a negative fresh gas balance), one for low surplus (the desired condition), and one for high surplus. A bar on the graph indicates the current surplus. A tendency indicator displayed in the window indicates the surplus tendency: a right arrow for tending higher, and a left arrow for tending lower. See the diagrams below:

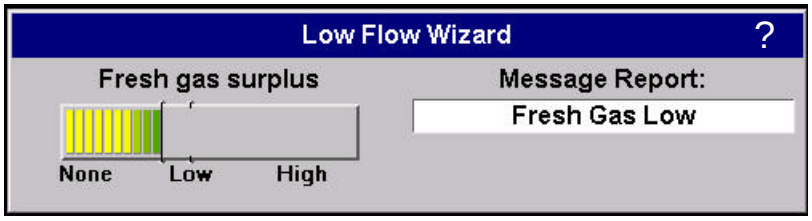

Figure 1: No surplus (a negative fresh gas balance)

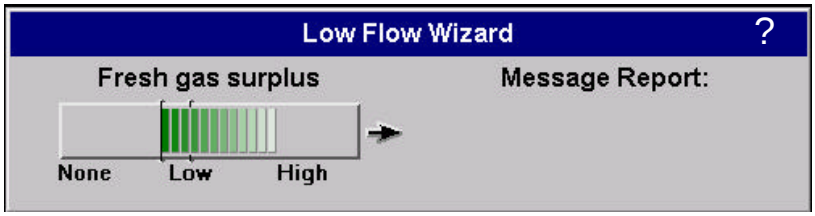

Figure 2: High surplus (fresh gas settings high)

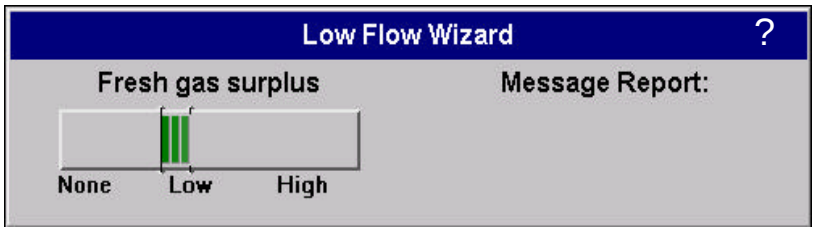

Figure 3: Desired level

Draeger Medical, Inc.
3135 Quarry Road
Telford, PA 18969
Tel: (215) 721-5403
(800) 523-6817
Fax: (215) 723-5934
Web: www.draegermedical.com

This feature will be available as a free upgrade for all new orders placed until December 31, 2000.

Description: Low Flow Wizard (new machine orders)
Part Number: 4116577
Price: $495.00

Description: Low Flow Wizard (after-market upgrade kit)
Part Number: 4116900
Price: $495.00 plus labor and travel

More detailed information is available in the Marketing Library database under product enhancements.

If you have any questions or require further information, please contact John Gotzon at x2619.